


Novel technique increases detection rate in screening mammography

February 4 2014

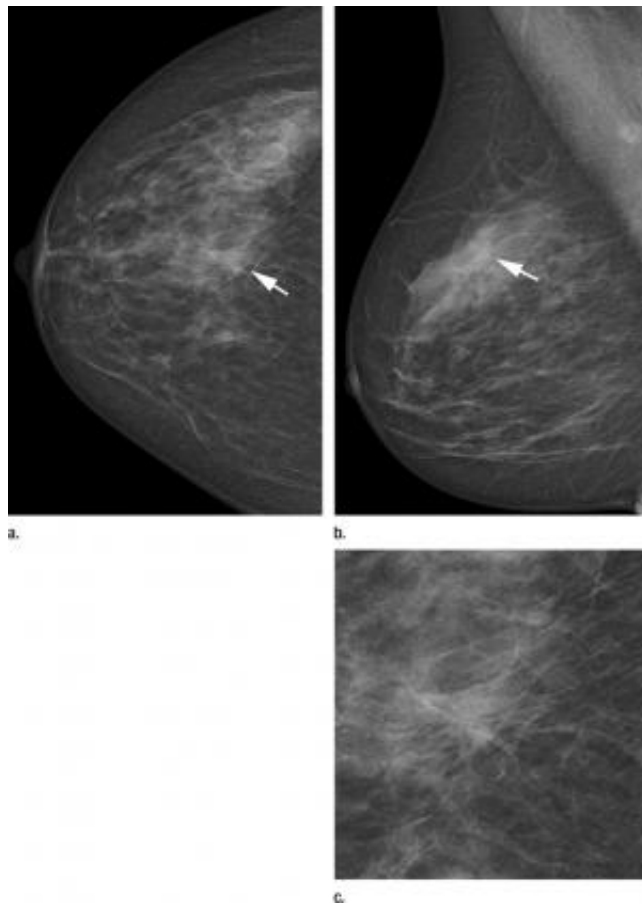


This shows two-view screening mammograms obtained with the DR photon-counting system show a spiculated mass in the right upper quadrants (arrow). The diagnosis was invasive ductal carcinoma, 8 mm in diameter, as seen on the (a) right craniocaudal image, (b) right mediolateral oblique image, and (c) zoomed in craniocaudal image of the lesion. Credit: Radiological Society of North America

Digital mammography screening with new photon-counting technique offers high diagnostic performance, according to a study published online in the journal *Radiology*.

As mammography screening has shifted to digital technology, a range of computed radiography (CR) and direct radiography (DR) systems have emerged. The photon-counting technique is a promising DR approach that uses a unique detector to decrease scattered radiation and noise, enabling dose reduction and making it a promising tool for screening.

"In population-based mammography screening, dose reducing techniques that don't compromise outcome parameters are desirable," said Walter Heindel, M.D., from the Department of Clinical Radiology at the University Hospital Muenster in Muenster, Germany.

For the study, Dr. Heindel and colleagues analyzed data from the [mammography screening](#) program in North Rhine-Westphalia, the most populous state in Germany. They compared the screening performance of a DR photon-counting scan system with those of statewide operating screening units using different digital technologies. During the study period (2009 – 2010), 13,312 women were examined using the photon-counting system, and 993,822 women were screened with either CR or DR systems alone.

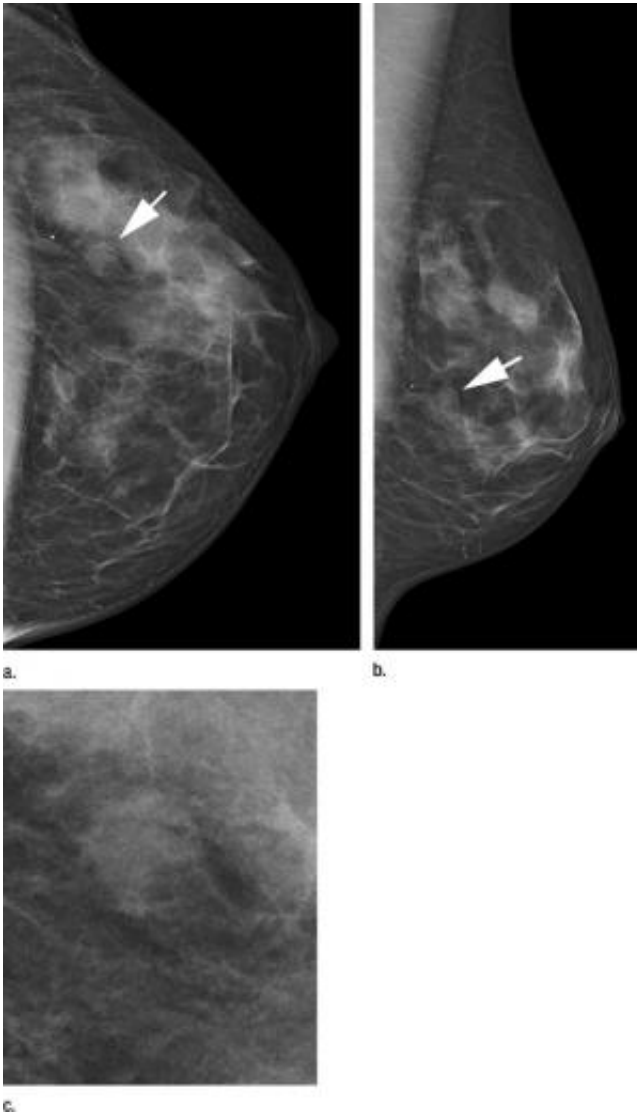

Two-view screening mammograms obtained with the DR photoncounting system show an indistinct mass in the left lower outer quadrant (arrow). The diagnosis was invasive ductal carcinoma, 7 mm in diameter, as seen on the (a) left craniocaudal image, (b) left mediolateral oblique image, and (c) zoomed in craniocaudal image of the lesion. Credit: Radiological Society of North America

The DR photon-counting scan system had a cancer detection rate of 0.76 percent for subsequent screening, compared with 0.59 percent for the other screening units. The recall rate was 5.4 percent for the photon-


counting method and 3.4 percent for the other methods.

"The higher cancer detection resulting from the use of the DR photon-counting scan system is due to high detection of both small, invasive cancers and ductal carcinoma in situ," Dr. Heindel said.

The photon-counting technique had almost twice the detection rate of other methods for ductal carcinoma in situ (DCIS), an early, noninvasive form of disease. It had a higher DCIS detection rate than the statewide units and the conventional DR subgroup.

In addition, the mean average glandular radiation dose of the DR photon-counting scan system was significantly lower than the conventional DR systems with the individually used parameters of the automatic exposure control.

The study's large size distinguishes it from previous studies that compared the DR photon-counting scan system's performance with other approaches.

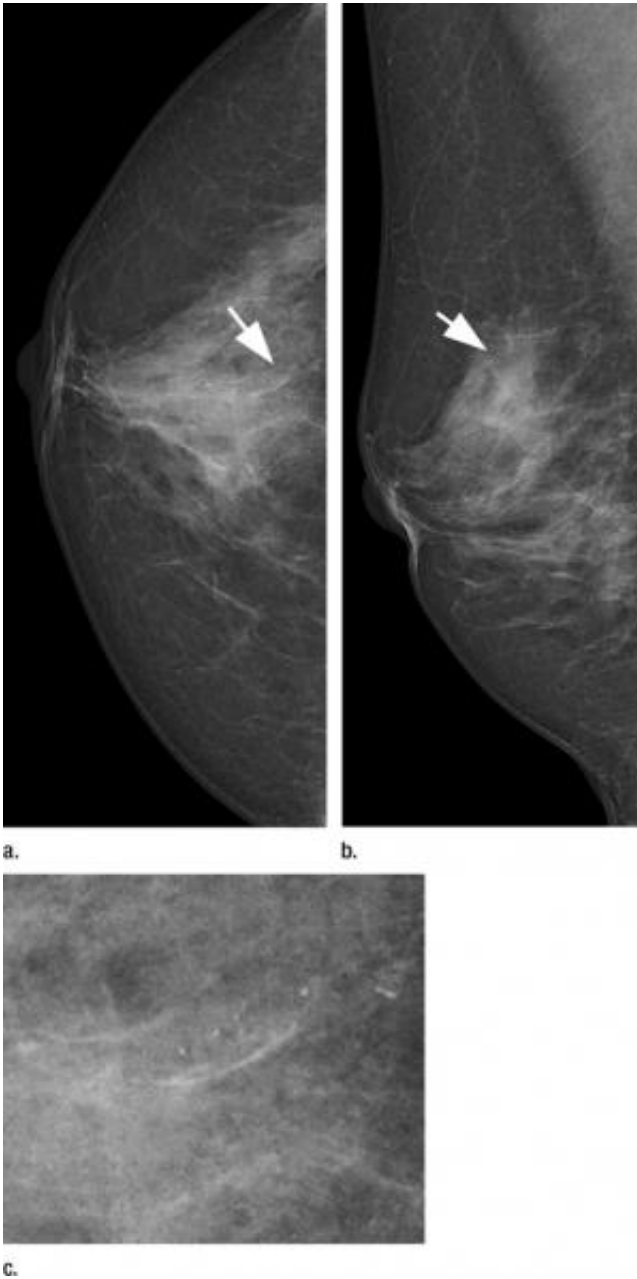

Two-view screening mammograms obtained with the DR photoncounting system show pleomorphic calcifications in a linear distribution in the right upper quadrants (arrow). The diagnosis was DCIS, as depicted on the (a) right craniocaudal image, (b) right mediolateral oblique image, and (c) zoomed in craniocaudal image of the lesion. Credit: Radiological Society of North America

"To our knowledge, the study is different from previous ones as we examined the performance of the DR photon-counting scan mammography on a larger database with consideration of multiple parameters of screening," said study coauthor Stefanie Weigel, M.D., from the University Hospital Muenster.

The photon-counting technique also offers lateral dose modulation during the image acquisition, which can help account for differences in breast density. Cancer often is more difficult to detect in women with dense breasts.

"The innovative photon-counting technique offers further research potential," Dr. Heindel said. "One future research direction is the application of spectral imaging for quantification of breast glandular tissue, addressing the problem of breast density."

More information: "Digital Mammography Screening with Photon-counting Technique: Can a High Diagnostic Performance Be Realized at Low Mean Glandular Dose?" *Radiology*, 2014.

Provided by Radiological Society of North America

Citation: Novel technique increases detection rate in screening mammography (2014, February 4) retrieved 5 May 2024 from

<https://medicalxpress.com/news/2014-02-technique-screening-mammography.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
--