


# High-speed 'label-free' imaging could reveal dangerous plaques

November 4 2014, by Emil Venere

---

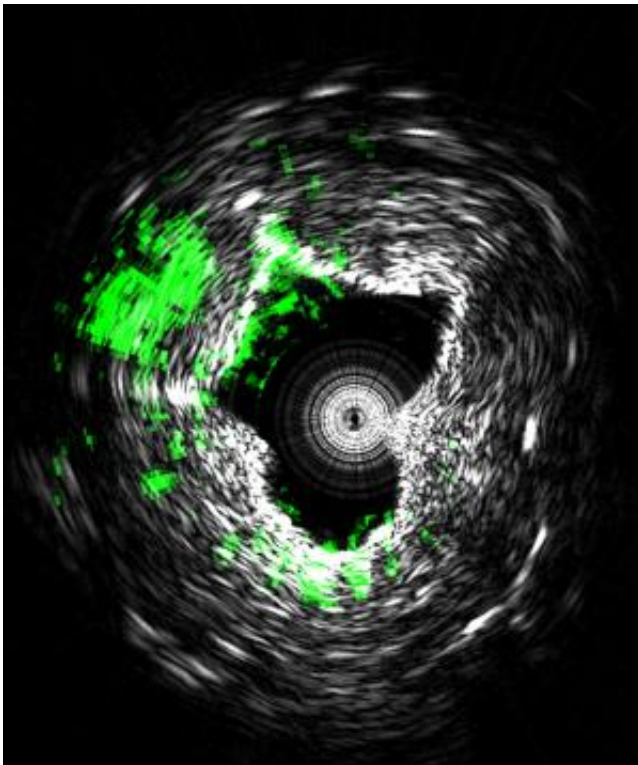

This image is taken using a new type of medical imaging technology that could diagnose cardiovascular disease by measuring ultrasound signals from molecules exposed to a fast-pulsing laser. The system, called intravascular photoacoustic imaging, takes precise three-dimensional images of plaques lining arteries and identifies deposits that are likely to rupture and cause heart attacks. This cross-sectional view of an artery shows lipids (green) deposited inside the arterial wall. Black and white indicate contrast showing the cross-sectional geometry. Credit: Purdue University Weldon School of Biomedical Engineering image/Ji-Xin Cheng

(Medical Xpress)—Researchers are close to commercializing a new type of medical imaging technology that could diagnose cardiovascular disease by measuring ultrasound signals from molecules exposed to a fast-pulsing laser.

The system takes precise three-dimensional images of plaques lining arteries and identifies deposits that are likely to rupture and cause heart attacks, said Ji-Xin Cheng (pronounced Jee-Shin), a professor in Purdue University's Weldon School of Biomedical Engineering and Department of Chemistry.

The imaging reveals the presence of carbon-hydrogen bonds making up [lipid molecules](#) in arterial plaques that cause heart disease. Research findings are detailed in a paper appearing online Tuesday (Nov. 4) in the Nature journal *Scientific Reports*.

"This allows us to see the exact nature of [plaque formation](#) in the walls of arteries so we can define whether plaque is going to rupture," said Michael Sturek, co-author of the paper and a professor and chair of the Department of Cellular & Integrative Physiology at Indiana University School of Medicine. "Some plaques are more dangerous than others, but one needs to know the chemical makeup of the blood vessel wall to determine which ones are at risk of rupturing."

Research in the area has been hindered by the inability to perform high-speed imaging in tissue. The researchers solved the problem by developing a Raman laser using a laser that produces 2,000 pulses per second, each pulse capable of generating an image, representing a 100-fold increase in the imaging speed of the new technology, called intravascular photoacoustic imaging.

"This innovation represents a big step toward advancing this technology to the clinical setting," Cheng said.

The paper was authored by researchers from Purdue, Indiana University School of Medicine, the University of California, Davis, the University of California, Irvine, and startup company Spectral Energy.

The imaging technique is "label free," meaning it does not require samples to be marked with dyes, making it appealing for diagnostic applications.

The technology is being commercialized by the company Vibronix Inc., co-founded by Cheng and Purdue postdoctoral research associate Pu Wang.

The laser, which pulses in the near-infrared range of the spectrum, causes tissue to heat and expand locally, generating pressure waves at the ultrasound frequency that can be picked up with a device called a transducer.

The paper was authored by Wang; USC graduate student Teng Ma; Purdue research scientist Mikhail N. Slipchenko; USC graduate student Shanshan Liang; Purdue graduate student Jie Hui; K. Kirk Shung, director of the Ultrasonic Transducer Resource Center at USC; Sukesh Roy, CEO of Spectral Energy LLC in Dayton, Ohio; Sturek; USC researcher Qifa Zhou; Zhongping Chen, a researcher at UC Irvine; and Cheng.

The system is small enough to be incorporated into an endoscope to put into blood vessels using a catheter, said Cheng.

The near-infrared laser causes enough heating to generate ultrasound but not enough to damage the tissues. The research was conducted with intact pig tissue and will expand to research with live animals and then clinical studies with humans.

The Purdue Office of Technology Commercialization has filed a U.S. patent application.

**More information:** High-speed Intravascular Photoacoustic Imaging of Lipid-laden Atherosclerotic Plaque Enabled by a 2-kHz Barium Nitrite Raman Laser, *Scientific Reports*, 2014.

Provided by Purdue University

Citation: High-speed 'label-free' imaging could reveal dangerous plaques (2014, November 4) retrieved 8 September 2024 from <https://medicalxpress.com/news/2014-11-high-speed-label-free-imaging-reveal-dangerous.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.