


# Target-vessel failure rate similar for scaffold, stent in PCI

March 30 2017

---

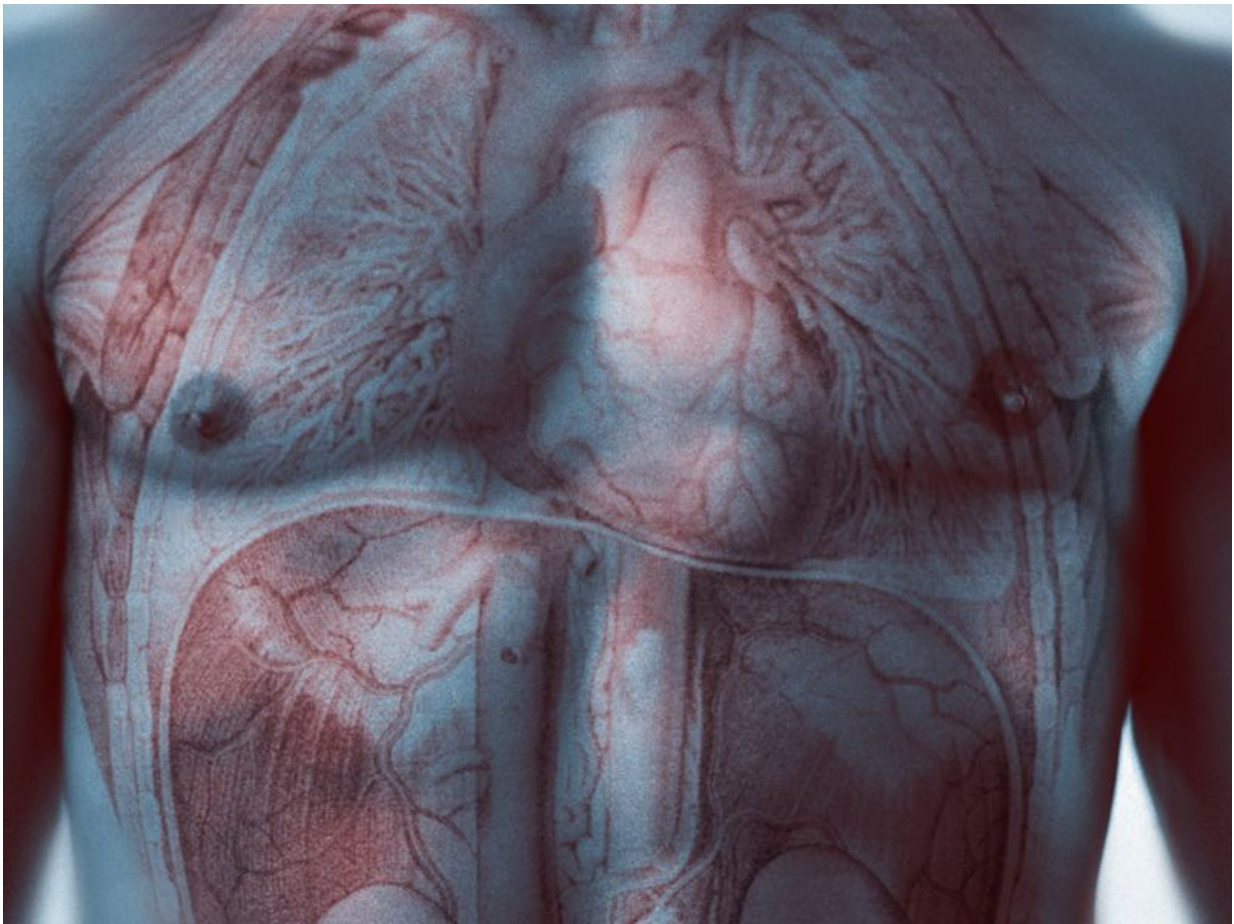

(HealthDay)—For patients undergoing percutaneous coronary

intervention (PCI), the rate of target-vessel failure does not differ significantly for those receiving a bioresorbable vascular scaffold or a metallic stent, according to a study published online March 29 in the *New England Journal of Medicine*.

Joanna J. Wykrzykowska, M.D., Ph.D., from the Academic Medical Center-University of Amsterdam, and colleagues randomized [patients](#) undergoing PCI to receive a bioresorbable vascular scaffold or a metallic stent (924 and 921 patients, respectively). Target-vessel failure (a composite of cardiac death, target-vessel myocardial infarction, or target-vessel revascularization) was assessed as the primary end point.

The researchers found that the two-year cumulative event rates for target-vessel failure were 11.7 and 10.7 percent in the scaffold and stent groups, respectively (hazard ratio, 1.12; 95 percent confidence interval, 0.85 to 1.48;  $P = 0.43$ ). The two-year cumulative event rates were 2.0 and 2.7 percent, respectively, for [cardiac death](#); 5.5 and 3.2 percent, respectively, for target-vessel myocardial infarction, and 8.7 and 7.5 percent, respectively, for target-vessel revascularization. The two-year cumulative event rates were 3.5 and 0.9 percent for the scaffold and stent groups, respectively, for definite or probable device thrombosis (hazard ratio, 3.87; 95 percent confidence interval, 1.78 to 8.42;  $P$

"There was no significant difference in the rate of target-vessel failure between the patients who received a bioresorbable scaffold and the patients who received a metallic stent," the authors write.

The study was funded by Abbott Vascular.

**More information:** [Abstract](#)  
[Full Text](#)  
[Editorial](#)

Copyright © 2017 [HealthDay](#). All rights reserved.

Citation: Target-vessel failure rate similar for scaffold, stent in PCI (2017, March 30) retrieved 1 May 2024 from <https://medicalxpress.com/news/2017-03-target-vessel-failure-similar-scaffold-stent.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.