


GAT values more discordant than DCT measures in glaucoma

May 17 2017

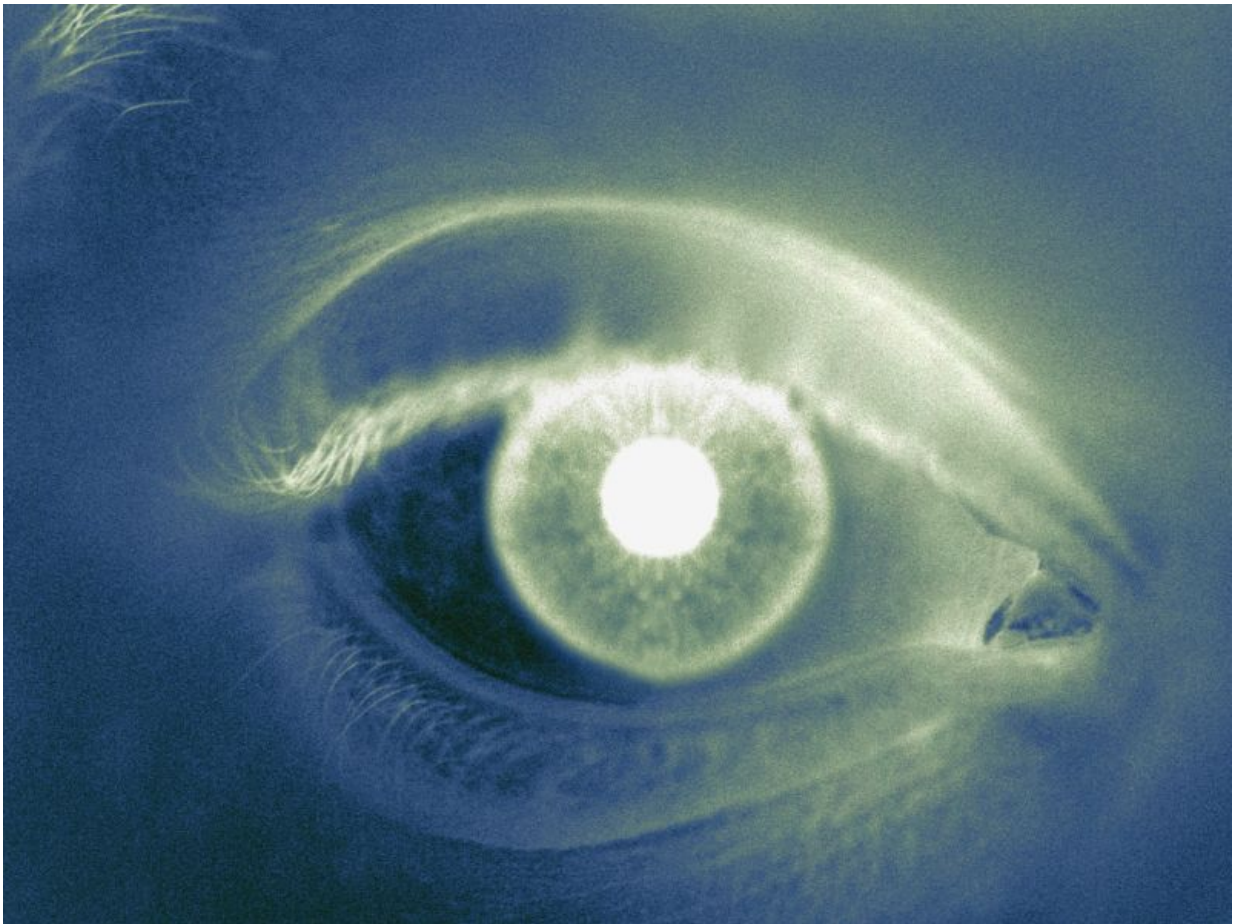

(HealthDay)—Conventional Goldmann applanation tonometry (GAT)

values for intraocular pressure (IOP) are significantly discordant compared with Pascal dynamic contour tonometry (DCT) measurements in patients with thin corneas and advanced glaucoma, according to a study published online May 11 in *JAMA Ophthalmology*.

Josephine Wachtl, from the University Hospital Zurich, and colleagues conducted a prospective cross-sectional case series among 112 white patients with [glaucoma](#). The authors performed IOP measurements with GAT and DCT and examined the difference between corrected and conventional GAT and DCT measurements.

The researchers found that the mean IOP was 20.3 and 17.0 mm Hg as measured by DCT and GAT, respectively, with a mean discordance between measures of -3.3 mmHg. Compared with DCT, the five corrected GAT values ranged from -2.7 to -5.4 mm Hg. The mean result of the Dresdner correction [formula](#) was 17.6 mm Hg, which was closer to the DCT than the GAT measurement. There was a mean Glaucoma Severity Score of 4.7. A positive correlation was seen for uncorrected discordance ($IOP_{DCT} - IOP_{GAT}$) with the Glaucoma Severity Score ($r_s = 0.33$), and a negative correlation with central corneal thickness ($r_s = -0.22$).

"Application of GAT-based correction formulas involves a possible risk of creating an even greater number of unpredictable measurement errors," the authors write. "Hence, we advise with caution, especially pertaining to eyes with thin corneas, to not place reliance on GAT readings, and abandon any correction formula."

More information: [Abstract/Full Text \(subscription or payment may be required\)](#)

[Editorial \(subscription or payment may be required\)](#)

Copyright © 2017 [HealthDay](#). All rights reserved.

Citation: GAT values more discordant than DCT measures in glaucoma (2017, May 17) retrieved 5 May 2024 from

<https://medicalxpress.com/news/2017-05-gat-values-discordant-dct-glaucoma.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.