


# A delicate crossing: Controller developed to open the blood-brain barrier with precision

November 15 2017

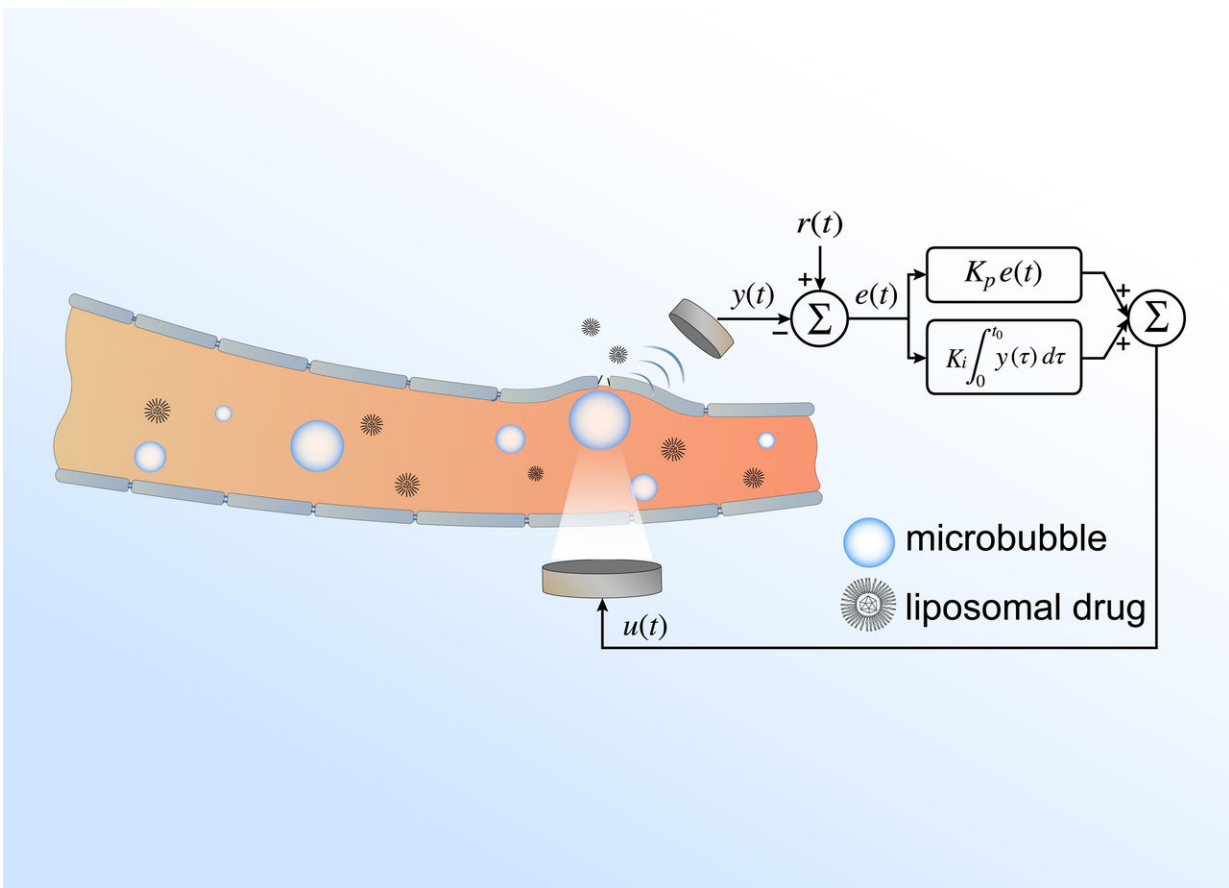

Representation of the drug delivery system. Serving as the acoustic indicator of drug delivery dosage, the microbubble emission signal  $y(t)$  is used to find the expected controller output  $u(t)$  which is fed back to help control ultrasound transducer transmission. Credit: Tao Sun, Brigham and Women's Hospital

The blood-brain barrier - the semi-permeable membrane that surrounds the brain - offers important protection for a delicate organ, but in some cases, clinicians need to get past the barrier to deliver vital drugs to treat the brain. Researchers at Brigham and Women's Hospital are investigating a way to temporarily loosen the blood-brain barrier to deliver drugs with the assistance of microbubbles. In a new advancement, they have developed a system in preclinical models that offers a finer degree of control - and, therefore, safety - in opening the barrier. Their findings are published this week in *The Proceedings of the National Academy of Sciences*.

"We want to be able to monitor our ability to open the [blood-brain barrier](#) in real-time by listening to echoes - this could give us immediate information on the stability of the microbubbles oscillations and give us fast, real-time control and analysis," said lead author Tao Sun, a PhD candidate in the labs of co-authors Nathan McDannold, PhD, in the Focused Ultrasound Laboratory in the Department of Radiology at BWH, and Eric Miller, PhD, chair and professor in the Department of Electrical and Computer Engineering at Tufts."

McDannold and his colleagues have been working for years on using focused ultrasound and microbubbles to disrupt the blood-[brain](#) barrier and deliver drugs to the brain. However, a major challenge for translating research advancements in this area into clinical impact has been a lack of a reliable way to get instantaneous feedback on how well microbubbles are vibrating inside the brain. Microbubbles can help temporarily open the blood-brain barrier without incision or radiation, but if these bubbles destabilize and collapse, they can damage the critical vasculature in the brain.

In the lab, the research team used a rat model to develop a closed-loop controller - a device that can give them a metaphorical window into the brain. By placing sensors on the outside of the brain that act like

secondary microphones, the research team could listen to ultrasound echoes bouncing off the [microbubbles](#) to determine how stable the bubbles were. They could then tune and adjust their ultrasound input instantly to stabilize the bubbles, excite them to open the [barrier](#), and deliver a drug of a predefined dose, while maintaining safe [ultrasound](#) exposure. The team tested the approach in healthy rats as well as an animal model of glioma brain cancer.

Further research will be needed to adapt the technique for humans, but the approach could offer improved safety and efficacy control for human clinical trials, which are now underway in Canada.

**More information:** Tao Sun et al, Closed-loop control of targeted ultrasound drug delivery across the blood–brain/tumor barriers in a rat glioma model, *Proceedings of the National Academy of Sciences* (2017). [DOI: 10.1073/pnas.1713328114](https://doi.org/10.1073/pnas.1713328114)

Provided by Brigham and Women's Hospital

Citation: A delicate crossing: Controller developed to open the blood-brain barrier with precision (2017, November 15) retrieved 5 May 2024 from <https://medicalxpress.com/news/2017-11-delicate-blood-brain-barrier-precision.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
--