


Contrast-enhanced ultrasound no aid for metastasis detection

December 15 2017

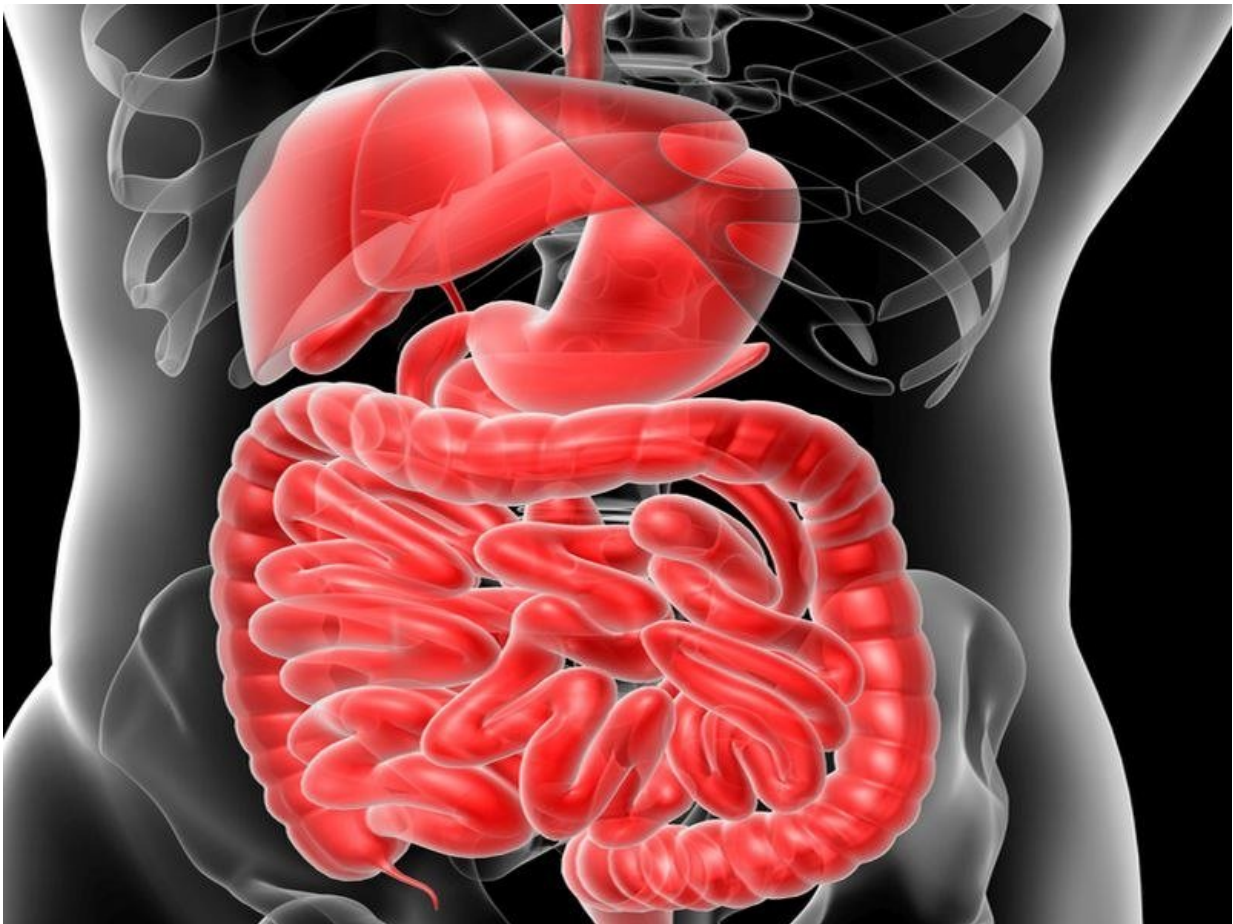

(HealthDay)—Contrast-enhanced laparoscopic ultrasonography (CE-

LUS) does not appear to increase the detection rate of liver metastasis during robotic-assisted surgery for primary colorectal cancer (CRC), according to a study published online Nov. 13 in the *Journal of Clinical Ultrasound*.

Signe Bremholm Ellebæk, M.D., from Odense University Hospital in Denmark, and colleagues assessed the potential clinical value of CE-LUS as a [screening tool](#) for [liver metastases](#) during robotic-assisted surgery for primary CRC among 50 consecutive patients.

The researchers found that patients were equally distributed between stage I, II, and III classification. CE-LUS did not detect any [liver metastasis](#), as was confirmed by follow-up using contrast-enhanced computed tomography imaging at three and 12 months postoperatively. CE-LUS was easy to perform and no complications were reported.

"The use of CE-LUS as a screening modality for detection of liver metastasis cannot be recommended based on this study, but larger controlled studies on high-risk patients seem relevant," the authors write.

More information: [Abstract](#)
[Full Text \(subscription or payment may be required\)](#)

Copyright © 2017 [HealthDay](#). All rights reserved.

Citation: Contrast-enhanced ultrasound no aid for metastasis detection (2017, December 15) retrieved 6 May 2024 from <https://medicalxpress.com/news/2017-12-contrast-enhanced-ultrasound-aid-metastasis.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.
