


# Device to corral viable sperm may speed IVF process

September 10 2018, by Blaine Friedlander

---

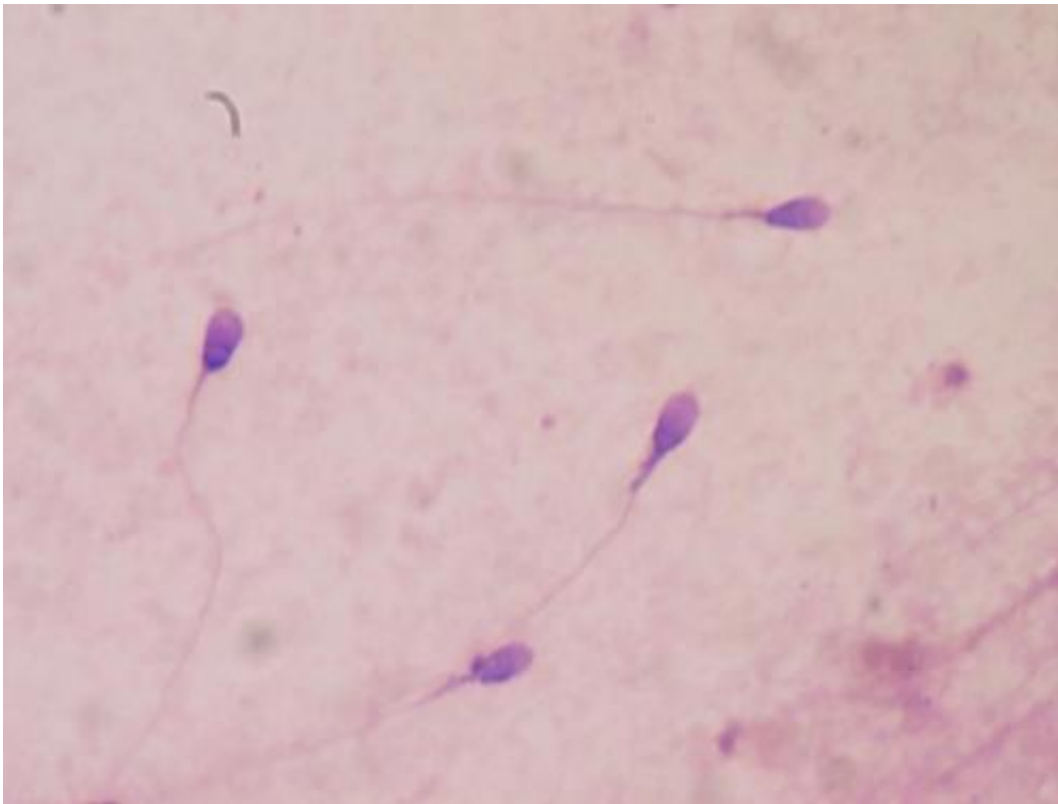

Human sperm stained for semen quality testing in the clinical laboratory. Credit: Bobjgalindo/Wikipedia

For couples hoping for a baby via in vitro fertilization, chances have improved. A process that once took hours now takes minutes: Cornell University scientists have created a microfluidic device that quickly corrals strong and speedy sperm viable for fertilization.

Conventional methods to separate vigorous, motile sperm is tedious and may take up to several hours to perform. "Trying to find the highly motile sperm has been difficult to do, but this improves the chances of insemination," said chemist Alireza Abbaspourrad, Cornell's Yongkeun Joh Assistant Professor of Food Chemistry and Ingredient Technology.

Taking advantage of sperm's ability to go against the flow—a process called rheotaxis—Abbaspourrad, Soon Hon Cheong, Ph.D., assistant professor at Cornell's College of Veterinary Medicine, and Meisam Zaferani, a doctoral student in the field of chemistry, have devised a [microfluidic](#) channel through which the sperm swim. They added a microscopic corral—shaped like a "C—that features a retaining wall that attracts the strongest swimmers.

"The older method is tedious, time-consuming and not efficient. It's the time that laboratory technicians and physicians expend that makes the process expensive," said Abbaspourrad. "With this method, it's five minutes instead of several hours."

The [microfluidic device](#) is simple to use: Rheotaxis is the key. "Here, we took advantage of sperm's natural tendency to redirect against fluid flow, once the sperm reach a certain velocity," said Cheong. "Once the sperm detect interference, they can use it to swim upstream. That's when we can trap them. We could separate the good sperm from the not-so-strong in a reasonably elegant way. We are able to fine-tune our selection process."

Zaferani said that these findings represent a broad range of applications beyond humans, such as using the device to separate motile bovine sperm for the dairy and beef industries. "The unprecedented efficiency of our device in comparison to previous studies and its benign, passive nature make it favorable for [sperm](#) separation," he said

The study, "Rheotaxis-Based Separation of Sperm with Progressive Motility Using a Microfluidic Corral System," published in the *Proceedings of the National Academy of Sciences* July 30.

**More information:** Meisam Zaferani et al, Rheotaxis-based separation of sperm with progressive motility using a microfluidic corral system, *Proceedings of the National Academy of Sciences* (2018). [DOI: 10.1073/pnas.1800819115](https://doi.org/10.1073/pnas.1800819115)

Provided by Cornell University

Citation: Device to corral viable sperm may speed IVF process (2018, September 10) retrieved 18 April 2024 from <https://medicalxpress.com/news/2018-09-device-coral-viable-sperm-ivf.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.