


Miniaturized, light-adaptive, wireless dosimeters autonomously monitor exposure to electromagnetic radiation

January 3 2020, by Thamarasee Jeewandara

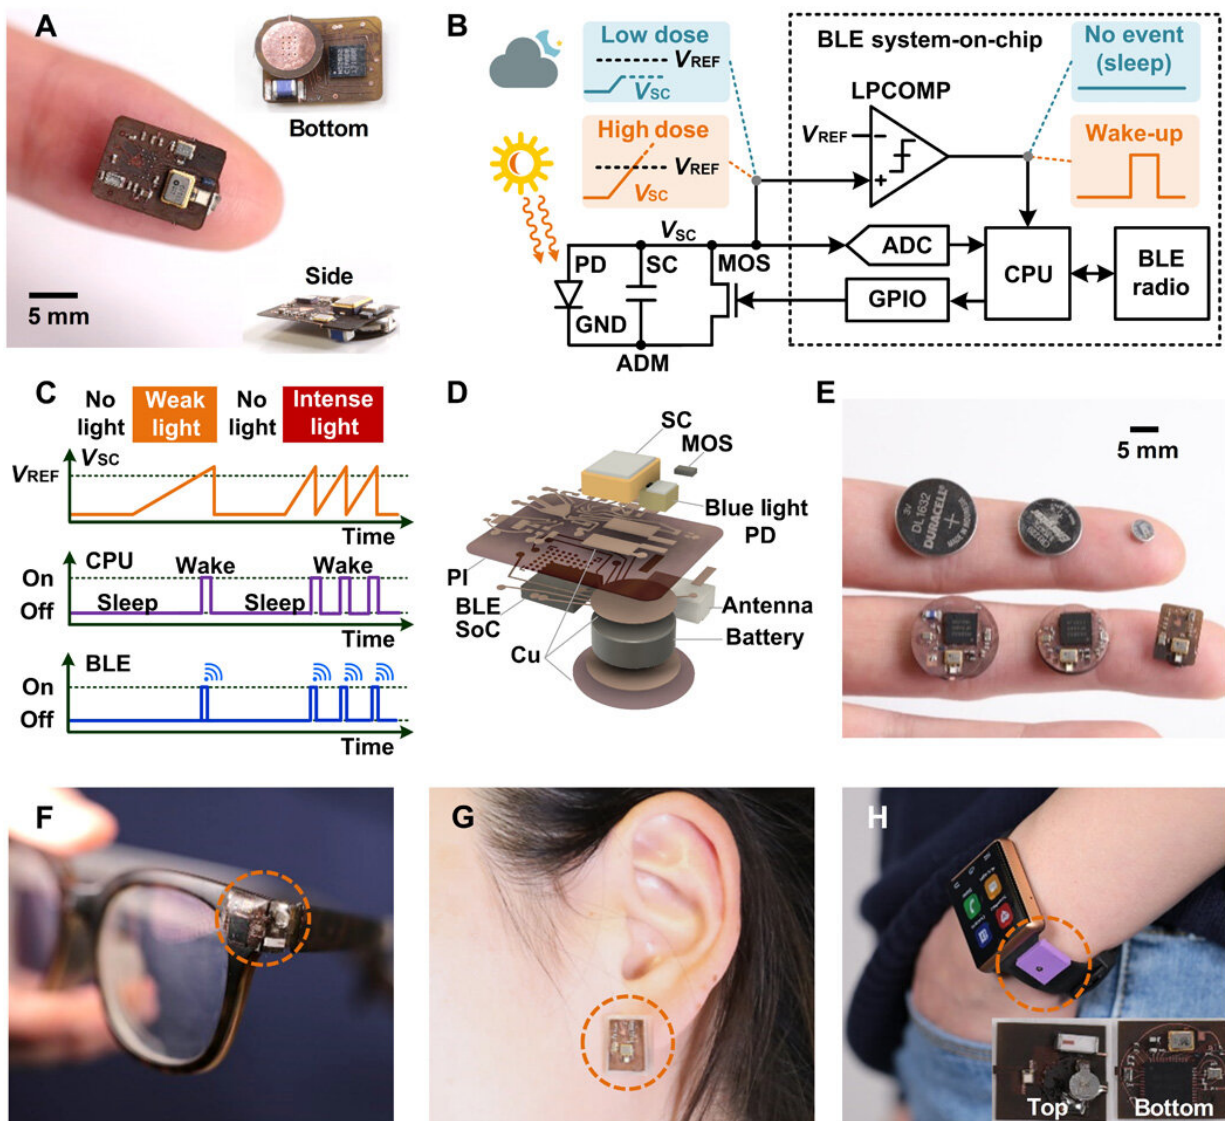


Ultralow-power, light-adaptive, wireless blue light dosimeter. (A) Photograph of a blue light dosimeter with BLE communication capabilities on the tip of an index finger. The insets show bottom and side views. (B) Circuit and block diagrams that illustrate accumulation mode, adaptive operation, and wireless interface to smartphones (BLE radio). The ADM, PD, SC, MOSFET, and low-power comparator (LPCOMP) are labeled ADM, PD, SC, MOS, and LPCOMP, respectively. VSC and VREF denotes the accumulated voltage on SC and the reference voltage of LPCOMP, respectively. ADC, analog-to-digital converter. (C) Illustration of VSC as a function of time during no light, weak light, and intense light exposure conditions and activity of central processing unit (CPU) and BLE radio at corresponding times. (D) Schematic, exploded view illustration of the constituent layers and components: BLE SoC, battery, MOSFET (MOS), SC, blue light photodiode (PD), copper interconnects [Cu/PI (polyimide)/Cu], and chip antenna. (E) Photographic image of three ultralow-power blue light dosimeters, next to respective batteries of capacities 140, 40, and 5.5 mA·hour (left to right). (F to H) Photographs of encapsulated sensors mounted on a pair of glasses, an earring, and a smart watch. Insets in (H) show top and bottom views of the unencapsulated device. Photo credit: Seung Yun Heo, Northwestern University. Credit: Science Advances, doi: 10.1126/sciadv.aay2462

Electromagnetic radiation (EMR) exposure from the sun and artificial lighting systems represent a health risk, therefore personalized methods for EMR [dosimetry](#) can guide people toward lifestyle behaviors that ensure healthy levels of exposure. In a recent report on *Science Advances*, Kyeongha Kwon and a research team in the departments of Biomedical Engineering, Statistics, Electronics Convergence Engineering and the Center for Advanced Regenerative Engineering in the U.S. and Korea developed a millimeter-scale, ultra-low-power digital dosimeter platform.

The device provided continuous EMS dosimetry using an autonomous mode, simultaneously with one or multiple wavelengths for time-managed, wireless consumer devices. The scientists included a single,

small button cell battery to support a multi-year life span, facilitated by a light-powered accumulation mode of detection and light-adaptive ultra-low-power circuit design. They employed field studies to demonstrate single- and multimodal dosimetry platforms and focused on monitoring short-wavelength [blue light](#) from indoor lightening, across to display systems, as well as detect ultraviolet/visible/infrared radiation from the sun.

Adverse influences of overexposure or underexposure to EMR can accumulate with [latent consequences](#); where excessive exposure to [ultraviolet radiation](#) (UVR) and blue light from the sun or emissions of tanning beds and cellphones, can have associated health risks. For instance, repetitive [keratinocyte](#) damage from chronic exposure to UVR is fundamental to cause skin cancer predominantly [in the United States](#). The shorter wavelengths of the visible spectrum (VIS) can generate [reactive oxygen species](#) in the skin to cause DNA damage, hyperpigmentation and inflammation, alongside collagen and elastin degradation to contribute to [photo-aging](#). Beyond specific thresholds, blue light can cause photochemical damage in retinal tissue to accelerate [age-related maculopathy](#) and modulate retinal control of the human circadian rhythm to [suppress melatonin secretion](#). Nevertheless, relative doses of UVR and VIS are essential to produce vitamin D and offer [immunomodulation](#), where insufficient exposure can lead to [seasonal affective disorder](#) that can be treated with bright light therapy.

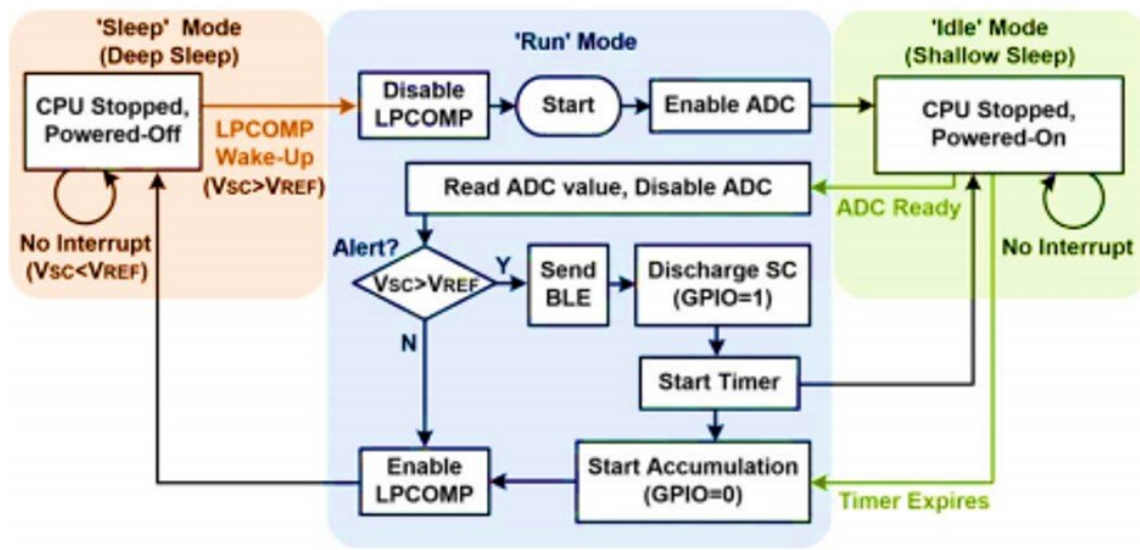

Flow diagram of BLE blue light sensing system using ultralow-power sleep/wake-up capability. When BLE operation starts, CPU triggers ADC sampling and goes into 'idle' mode (shallow sleep mode), which makes the entire BLE SoC, except ADC and Timer, wait in a halt status. When the ADC reports a ready interrupt, the CPU wakes up, reads the ADC value and compares the SC voltage (V_{SC}) against a preprogrammed reference voltage (V_{REF}). At low blue-light conditions, $V_{SC} < V_{REF}$, CPU alerts the user by sending BLE packets, starts discharging SC (sets GPIO as high voltage) and enters 'idle' mode. After a preprogrammed discharging duration (e.g. 5 s), CPU wakes up and finishes discharging (sets GPIO as low voltage) and goes in to 'sleep' mode. Credit: Science Advances, doi: 10.1126/sciadv.aay2462

Recent scientific proposals to detect personal information on wavelength-specific exposure to EMR can guide patient behavior to prevent adverse health results. Strategies include miniaturized, highly accurate dosimeters that explore a light-powered, continuous mode of detection [for battery-free operation](#). Researchers had used a miniaturized loop antenna to support near-field communication (NFC) as a digital wireless interface

during data acquisition but multi-millimeter-scale NFC (mm-NFC) devices are not automated, requiring active user engagement for data acquisition.

An ideal platform can offer autonomously remote wireless updates while retaining key features of the mm-NFC approach, which Kwon et al. used as a strategy, accompanied with an advanced light-adaptive electronic control circuit. The setup included an accumulation detection module (ADM) for dosimetry and a Bluetooth low energy (BLE) system on a chip (SoC) for wireless communication. As a key feature, the scientists built-in the ADM to directly measure continuous dose exposure without power consumption. In contrast, conventional digital approaches approximated dose through time integration across brief measurements of intensity using active, battery-powered electronics; where increased sampling frequency increased the accuracy but decreased the battery life. The ADM eliminated this trade-off to accomplish highly accurate dosimetry with extremely long intervals between active measurements.

The device remained in an ultra-low sleep mode ($\sim 0.4 \mu\text{A}$) in the absence of light while continuously monitoring dosage via the ADM. When the dose exceeded a threshold, the device briefly woke up ($\sim 10 \mu\text{A}$) to wirelessly transmit exposure data using BLE (Bluetooth low energy) protocols to a smartphone to then reset the ADM and quickly return to sleep mode. The work resulted in an exceptionally power efficient dosimeter with automatic regulation and communication capabilities without active user engagement. Kwon et al. aim to implement the device for blue light dosimetry and multispectral measurements in the UVR, blue and infrared (IR) regions of the spectrum, with proof-of-principle applications in [field trials](#) completed in this work.




TOP: Circuit and block diagrams that illustrate accumulation mode, adaptive operation, and wireless interface to smartphones Schematic, expanded view illustration of the constituent layers and components: BLE SoC, battery, MOSFET (MOS), SC, blue light photodiode (PD), copper interconnects [Cu/PI (polyimide)/Cu], and chip antenna. BOTTOM: Photographic image of three ultralow-power blue light dosimeters, next to respective batteries of capacities 140, 40, and 5.5 mA·hour (left to right). (F to H) Photographs of encapsulated sensors mounted on a pair of glasses, an earring, and a smart watch. Insets show top and bottom views of the unencapsulated device. Photo credit: Seung Yun Heo, Northwestern University. Credit: Science Advances, doi: 10.1126/sciadv.aay2462

The scientists explored the unique design features of blue light dosimetry with an estimated device operating lifetime of 1-2 years. They included a photodiode (PD), supercapacitor (SC) and metal oxide semiconductor field-effect transistor (MOSFET) within the ADM. Using the PD, Kwon et al. continuously and passively generated photocurrents with a magnitude directly and linearly proportional to the intensity of

exposed light. They arranged the SC in parallel with the PD to capture and store the resulting accumulated charge. They prevented excessive charge build up on the SC by connecting a gate of the MOSFET to a general-purpose input/output (GPIO) for programmable control of the current flow between the source and the drain of the MOSFET to trigger SC discharge.

Kwon et al. preprogrammed the reference voltage (V_{REF}), where the device remained in sleep mode unless conditions exceeded values to reduce average current consumption. The wake-up frequency of the setup increased with increasing irradiation in the wavelength range. The team programmed the dosage data into the memory of the BLE SoC (Bluetooth Low Energy System on a Chip) to prevent unexpected data loss due to wireless connection disruption. Kwon et al. used thin copper-based polyimide sheets processed with a laser cutting tool to engineer the device. The battery determined the size and weight of the resulting product and its operating lifetime. The scientists deployed miniaturized forms of the device on sunglass clips, earrings and wristbands for personalized EMR exposure detection.

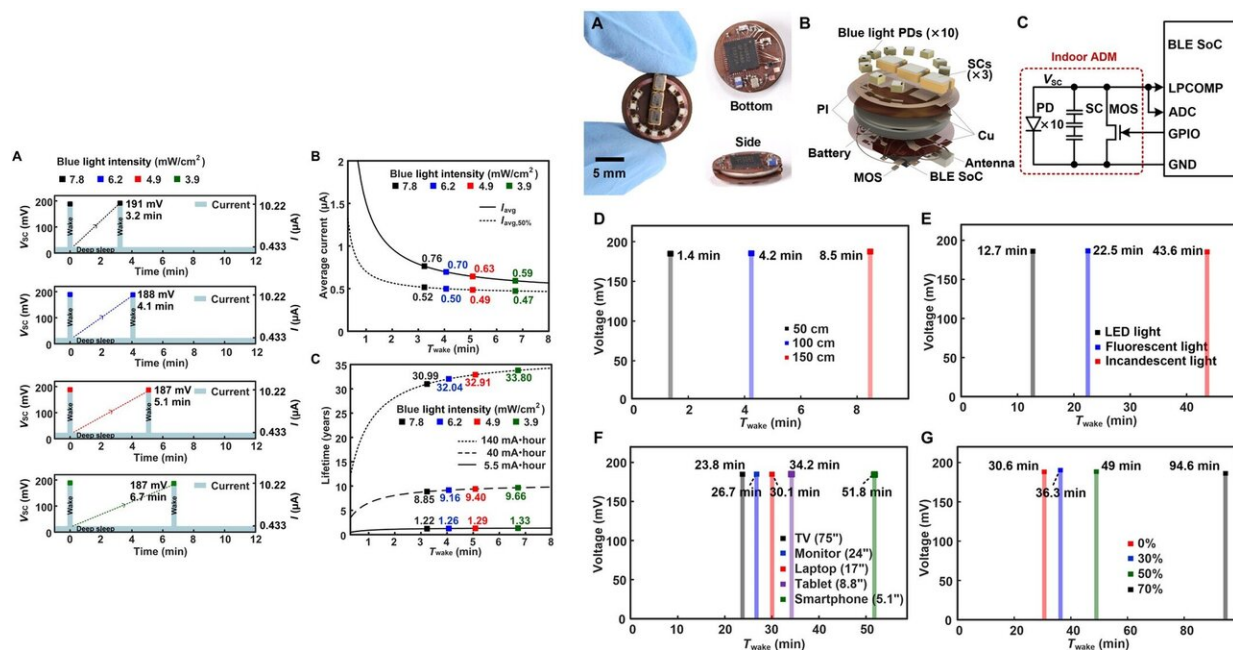



LEFT: Outdoor characterization and power consumption of blue light dosimeters. (A) Voltage outputs and current consumptions of an ultralow-power, blue light dosimeter ($n = 1$) exposed to blue light over time with constant intensity at four different intensities corresponding to low and moderate blue light conditions outdoors. The time intervals (T_{wake}) to “wake” the devices from a sleep state when exposed to blue light with constant intensity of different levels are indicated. (B) Average current consumption assuming continuous use (I_{avg}) and average current consumption assuming use corresponding to 50% of available daylight ($I_{\text{avg},50\%}$) as a function of T_{wake} . (C) Projected lifetime as a function of T_{wake} for batteries of capacities of 140, 40, and 5.5 mA·hour assuming use corresponding to 50% of available daylight: lifetime = battery capacity/ $I_{\text{avg},50\%}$. RIGHT: Indoor characterization of light-powered, accumulation mode detection blue light dosimeters. (A) Photograph of an indoor blue light dosimeter held between the fingertips. (B) Schematic, exploded view illustration of the constituent layers and components: BLE SoC, battery, a MOSFET (MOS), SCs ($\times 3$), blue light PDs ($\times 10$), copper interconnects (Cu/PI/Cu), and chip antenna. (C) Circuit and block diagrams of the system and its wireless interface to BLE-enabled devices for blue light monitoring indoors. (D to G) Voltage output and wake-up time interval of an indoor blue light dosimeter ($n = 1$) placed at a distance of 50, 100, and 150 cm from a white light phototherapy lamp (D), at a distance of 50 cm from artificial light sources (E), at a distance of 10 cm from display screens (F), and at a distance of 5 cm away from a tablet display equipped with 0, 30, 50, and 70% blue light blocking filter (G). The T_{wake} values are labeled. Photo credit: Seung Yun Heo, Northwestern University. Credit: Science Advances, doi: 10.1126/sciadv.aay2462

The team first designed blue light dosimeters for outdoor use. For runtime after wake-up events, the team took three time frames into consideration, which included T_{ADC} (time required for the ADC input voltage), T_{BLE} (time to transmit the sampled data via BLE) and T_{DSC} (preprogrammed time to fully discharge the SC), for a total of 6.56

seconds. They used on-chip data retention strategies to prevent data loss, where the BLE SoC maintained a 4-kilobyte static random access memory (SRAM). Kwon et al. programmed the device to store at least 10 measurements in the SRAM to transmit the entire dataset upon each wake-up event, when the phone was within communication range of the device.

The research team also developed blue light dosimeters for use indoors, since artificial lights and displays emit blue light to cause health risks after prolonged exposure. The setup was similar to outdoor dosimeters, with a higher collection of PDs (photodiodes) and SCs (supercapacitors) to increase the photocurrent and decrease storage capacity for increased sensitivity of the setup. The team obtained representative results from exposure to a variety of indoor light sources. The largest screen display belonged to the television, which emitted the most amount of blue light and smallest screen display to the smartphone radiating the least amount of blue light. The scientists used a commercial anti-blue light film in the experiments, which blocked approximately 17.5 percent of the radiation near 390 nm.

Kwon et al. subsequently constructed blue light dosimeters to simultaneously track exposure indoors and outdoors via an automated, wireless scheme that switched between parallel sensing circuits based on the presence (outdoors) or absence (indoors) of UVA radiation. The system updated the one-bit flag value at every wake-up event (indicating zero for indoor and one for outdoor exposure), passed the information to the user interface to activate indoor/outdoor ADM and re-enter sleep mode. The scientists assessed the most significant bit of the data obtained to calculate the exposure indoors and outdoors.

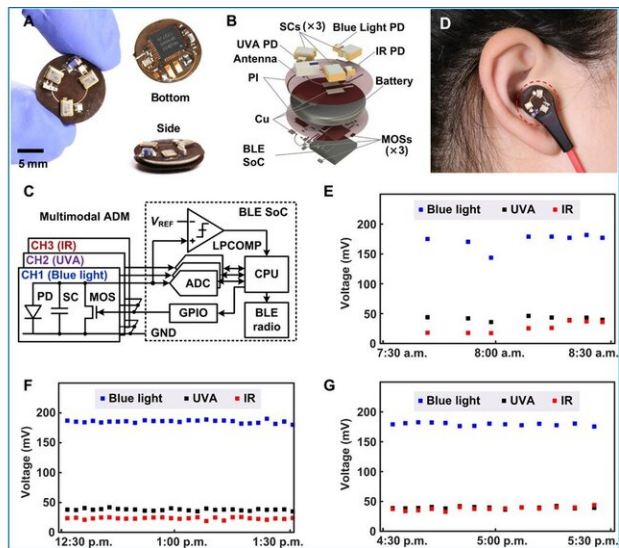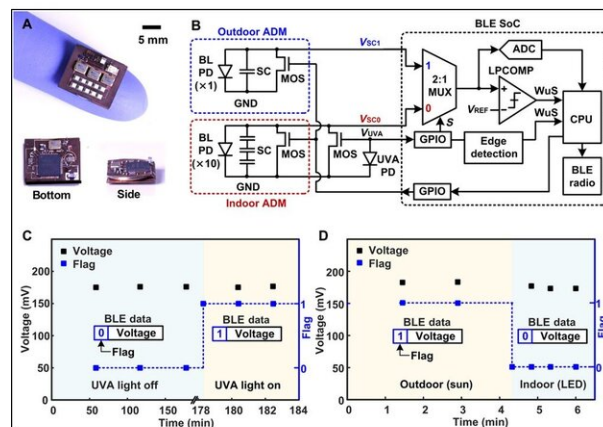

RIGHT: Outdoor/indoor dual-use blue light dosimeters with an automated, wireless sensitivity switching scheme. (A) Photographic image of a blue light dosimeter with an automated sensitivity switching scheme to allow monitoring of low-intensity blue light indoors and high-intensity blue light outdoors. (B) Circuit and block diagrams of the system with wireless switching scheme between outdoor and indoor sensing circuits based on the presence or absence of UVA irradiation. Blue light PD, MOSFET, SC, MUX, selection signal, the anode voltage of a UVA PD, and WuS are labeled BL PD, MOS, SC, MUX, S, VUVA, and WuS, respectively. (C) Voltage and 1-bit flag (0 for indoor and 1 for outdoor) outputs as a function of time without UVA exposure (blue) and with UVA exposure (yellow). (D) Voltage and 1-bit flag outputs as a function of time with daylight outdoors (yellow) and with a 60-LED ring light source (blue). Photo credit: Seung Yun Heo, Northwestern University. LEFT: Multichannel system: Dosimeters with capabilities for simultaneous measurements in the UVA, blue, and IR. (A) Photograph of an ultralow-power, three-channel, UVA/blue/IR light dosimeter held between the fingertips. (B) Schematic, exploded view illustration of the constituent layers and components: the BLE SoC, battery, MOSFETs (x3 MOS), SCs (x3 SC), UVA photodiode (UVA PD), blue light PD, IR PD, copper interconnects (Cu/PI/Cu), and chip antenna. (C) Circuit and block diagrams of the adaptive, accumulation mode of detection, and wireless interface to a remote BLE radio (i.e., smartphones). (D) Photographs of a multichannel sensor mounted on earphones. (E to G) Measurements obtained from a UVA/blue/IR light dosimeter ($n = 1$) as a function of time during

morning (E), noon (F), and afternoon (G) hours in Evanston, IL on April 2019. Photo credit: Seung Yun Heo, Northwestern University. Credit: Science Advances, doi: 10.1126/sciadv.aay2462

The team also developed a multichannel dosimeter for wavelengths in the UVA, blue and IR regions of the solar spectrum. They expanded the underlying designs and operating principles for simultaneous dosimetry of up to seven different wavelengths across the solar spectrum from UV to VIS and IR. Kwon et al. used a three-channel device to measure exposure dose and wirelessly transmit the data collected under specific conditions to a smartphone.

In this way, Kyeongha Kwon and colleagues combined adaptive circuit designs and accumulation detection schemes to continuously monitor personalized EMR exposure levels. The miniaturized, compact and wireless digital platforms gathered information across multiple wavelengths automatically, while continuously adjusting to surrounding conditions. The highly accurate, multimeter-scale systems functioned in an 'always on' state to facilitate multiyear lifetimes in practice. The resulting personalized information can be used to guide health behaviors. The device represents an ideal collection of features, including power management, battery replenishment, wearability and negligent user burden during data acquisition. The [frugal technology](#) and mass manufacturing capacity can offer large-scale dosimetry development and deployment to prevent risks of skin cancer, mood disorders, ocular damage and associated risks of EMR exposure.

More information: Kyeongha Kwon et al. Miniaturized, light-adaptive, wireless dosimeters autonomously monitor exposure to electromagnetic radiation, *Science Advances* (2019). [DOI: 10.1126/sciadv.aay2462](https://doi.org/10.1126/sciadv.aay2462)

Yunzhou Shi et al. Soft, stretchable, epidermal sensor with integrated electronics and photochemistry for measuring personal UV exposures, *PLOS ONE* (2018). [DOI: 10.1371/journal.pone.0190233](https://doi.org/10.1371/journal.pone.0190233)

Seung Yun Heo et al. Wireless, battery-free, flexible, miniaturized dosimeters monitor exposure to solar radiation and to light for phototherapy, *Science Translational Medicine* (2018). [DOI: 10.1126/scitranslmed.aau1643](https://doi.org/10.1126/scitranslmed.aau1643)

© 2020 Science X Network

Citation: Miniaturized, light-adaptive, wireless dosimeters autonomously monitor exposure to electromagnetic radiation (2020, January 3) retrieved 3 May 2024 from <https://medicalxpress.com/news/2020-01-miniaturized-light-adaptive-wireless-dosimeters-autonomously.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
--