

Detecting skin disorders based on tissue stiffness with a soft sensing device

May 28 2021



The research team designs a simple, miniature electromechanical device for high-precision and real-time evaluations of deep tissue stiffness. Credit: Dr Yu Xinge's team

By putting a piece of soft, strain-sensing sheet on the skin may be able to

detect skin disorders non-invasively and in real-time very soon. A research team co-led by a scientist from City University of Hong Kong (CityU) has designed a simple electromechanical device that can be used for deep tissue pathology diagnosis, such as psoriasis, in an automated and non-invasive fashion. The findings will lay a foundation for future applications in the clinical evaluation of skin cancers and or dermatology diseases.

The research is co-led by Dr Yu Xinge, Assistant Professor from CityU's Department of Biomedical Engineering, and scientists from and Northwestern University in the US. Their findings have been published in the science journal *Nature Biomedical Engineering*, titled "Miniaturized [electromechanical devices](#) for the characterization of the biomechanics of deep tissue."







Electromechanical systems that enable precise, rapid measurements of the stiffness of soft tissues of the human body can provide useful clinical information for monitoring, diagnosing and treating various pathologies, particularly those of the [skin](#). However, existing diagnostic evaluations, for example, magnetic resonance elastography, usually involve huge instruments at hospitals and trained practitioners. And the latest tissue stiffness-measuring technology based on sensing can only measure to superficial depths of upper skin, up to micrometer scale.

New device for real-time evaluations of deep tissue stiffness

To address the issue, the research team designed a simple, miniature electromechanical device for high-precision, real-time evaluations of deep tissue stiffness. The team used a miniature electromagnetic system that integrates a vibratory actuator and a soft strain-sensing sheet to monitor in [real-time](#) the Young's modulus, ie the tensile stiffness, of skin

and other soft biological tissues at depths of approximately 1 to 8 mm, depending on the sensor designs.

The team evaluated the device's performance with a range of synthetic and biological materials, such as hydrogels, pigskin and on various parts of human skin. "The lesions exhibited higher stiffness than those of the nearby skin, primarily due to differences in skin elasticity and hydration. These simple measurements have potential clinical significance in rapidly identifying and targeting skin lesions, with capabilities that complement those of recently reported methods for sensing mechanical properties at tissue surface (typically micrometer-scale)," explained Dr Yu. He pointed out that cancer tissue is typically stiffer or softer than normal tissue, and such difference can be used as diagnostic biomarker for a range of skin conditions, like skin cancer or tumors under the skin.

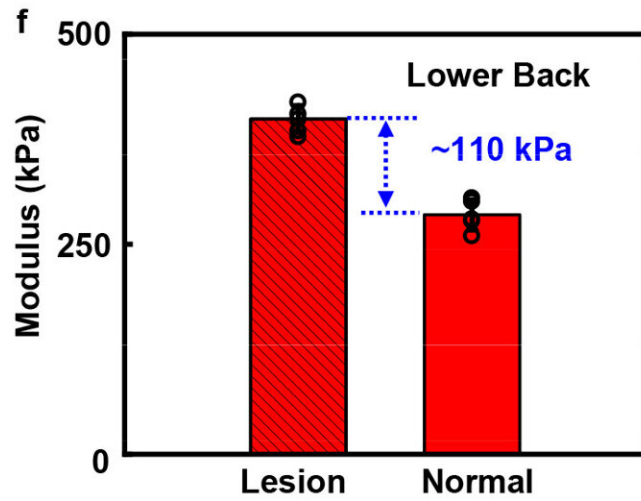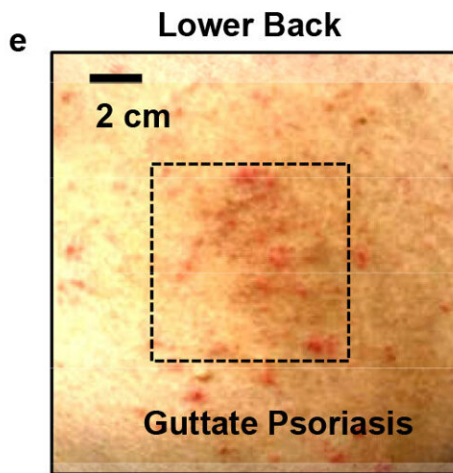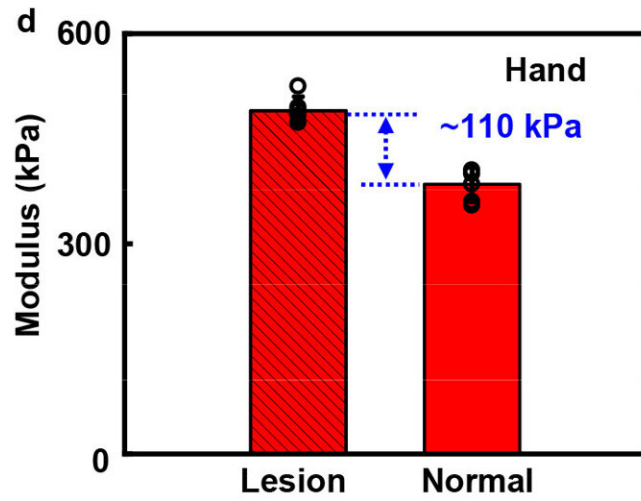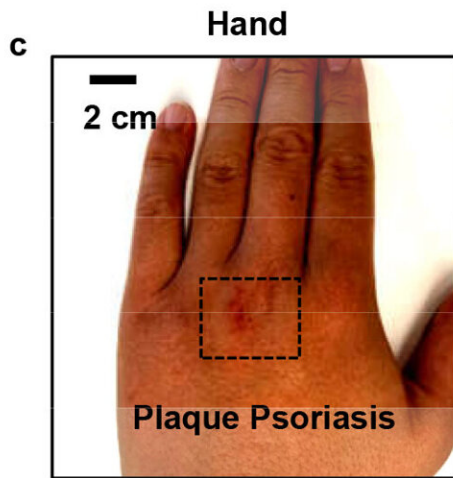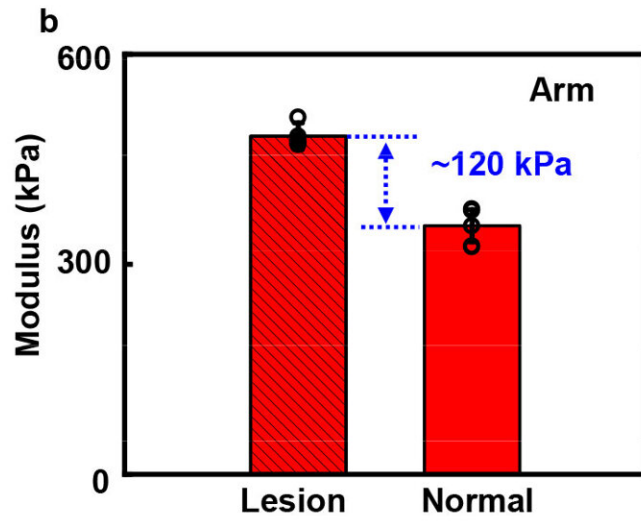
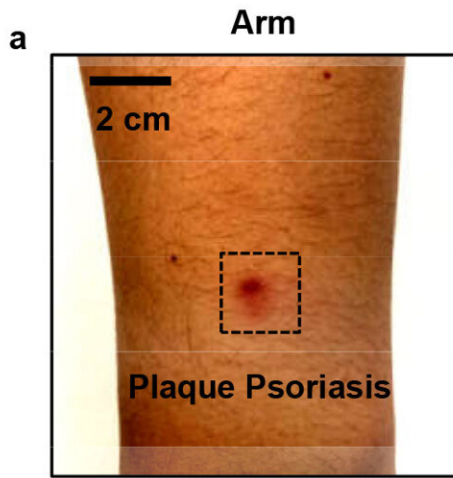


The team applies the device on the skin lesions associated with psoriasis on the arm (a), hand (c), lower back (e) and the unaffected skin. Figure b, d and f show the results of stiffness variations between unaffected skin and lesion regions. Credit: Song, E., Xie, Z., Bai, W. et al. / DOI : 10.1038/s41551-021-00723-y

A simple structure of the electromechanical device

The electromechanical device's thickness is only about 2.5 mm, and the contacting area is about 2 cm². It operated well on both hair-bearing and hairless areas of the skin. Its working mechanism is adapted from the basis of a skin-integrated haptic interface for virtual/augmented reality developed by Dr Yu and the collaborators from Northwestern University before.

The device works like this: after applying an alternating current through the copper coil, the magnet vibrates and creates pressures onto the bottom surface of the sensor. This would direct deformations that extend to millimeter-scale depths of [tissue](#), which leads to periodic variations in electrical resistance. Analyses of these responses by simultaneously measuring the voltage allows quantitative determination of the stiffness of the tissues. Each measurement could be done within one minute.

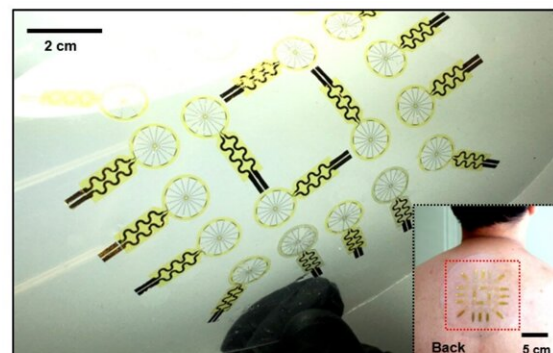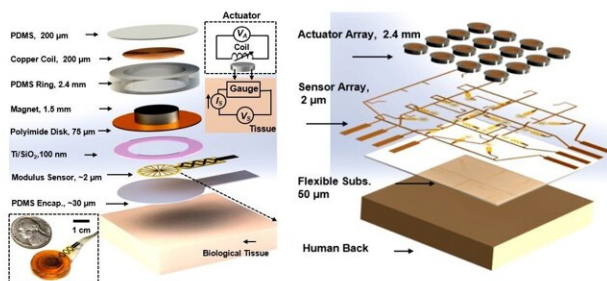

Schematic illustration of the mechanical actuators and sensors for quantitatively measuring the stiffness of biological surfaces. The lower-left inset shows the device is more or less the size of a US five-cent coin. And the other two pictures are the illustration of arrays of sensing device which support spatial mapping of tissue stiffness. Credit: Song, E., Xie, Z., Bai, W. et al. / DOI : [10.1038/s41551-021-00723-y](https://doi.org/10.1038/s41551-021-00723-y)

The team then conducted clinical studies on patients with skin disorders with their newly invented electromechanical device. The results indicated a potential for accurate targeting of lesions associated with psoriasis, showing the practical medical utility of the device. "The data produced can assist in diagnosis, treatment tracking and disease monitoring particularly for skin associated disorders such as skin cancer, as well as in aspects of aesthetic dermatology and of the recovery from surface wounds," said Dr Yu.

Dr Yu also pointed out that their device has the potential to be used for the evaluation of skin physical properties under various conditions such as aging, hydration loss or associated dermatological disorders. "In the near future, we believe this technology will allow people to monitor their skin health status anytime with a simple wearable [device](#)," said Dr Yu.

More information: Enming Song et al, Miniaturized electromechanical devices for the characterization of the biomechanics of deep tissue, *Nature Biomedical Engineering* (2021). [DOI: 10.1038/s41551-021-00723-y](https://doi.org/10.1038/s41551-021-00723-y)

Provided by City University of Hong Kong

Citation: Detecting skin disorders based on tissue stiffness with a soft sensing device (2021, May 28) retrieved 25 April 2024 from <https://medicalxpress.com/news/2021-05-skin-disorders-based-tissue-stiffness.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.