


A simple, low-cost LAMP-based device that can detect low concentrations of pathogens in patient samples

September 7 2023, by Bob Yirka

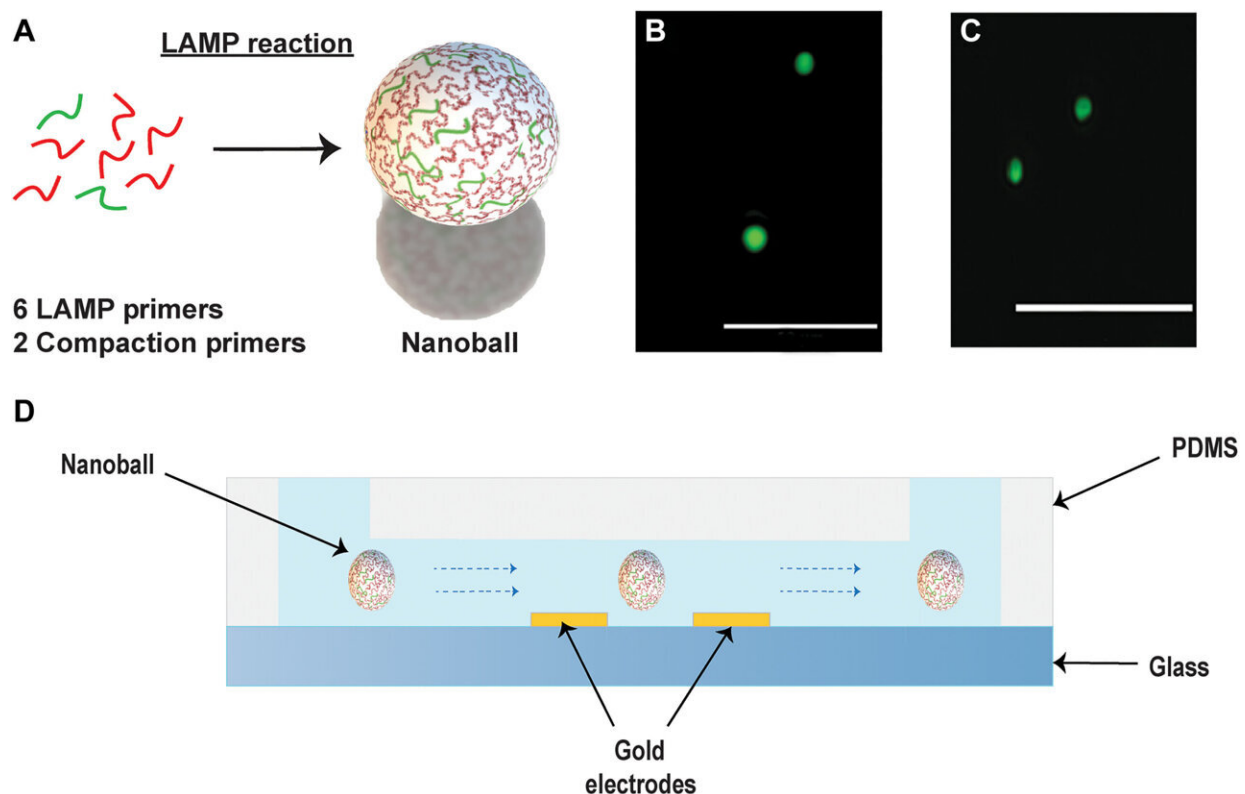

Electrical detection of DNA nanoballs. (A) Formation of DNA nanoball using six target-specific LAMP oligos and two compaction oligos. (B) Fluorescence image of DNA nanoballs. Scale bar, 10 μm . (C) Fluorescent image of 1 μM MyOne Dynabeads as size reference. Scale bar, 10 μm . (D) Passive flow of DNA nanoballs in a microfluidic chip made of PDMS on a glass substrate integrated with gold electrodes. The passage of DNA nanoballs through the gold

electrodes occludes the current path and disturbs the electric field formed between the gold electrodes. (E) A schematic illustrating the electronic readout system used for the microfluidic chip with integrated gold electrodes. Credit: *Science Advances* (2023). DOI: 10.1126/sciadv.adi4997

A team of microbiologists from Rutgers, The State University of New Jersey, the Karolinska Institutet, Yale University and Stanford University has developed a simple, low-cost LAMP-based device that can be used to detect low concentrations of pathogens in patient samples. The group describes the factors that went into developing the device in the journal *Science Advances*.

One of the lessons learned from the global pandemic was that there is a need for a low-cost, easy-to-use device that can detect a COVID-19 infection before the onset of symptoms. Isolating such people would prevent the spread of the disease. In this new effort, the research team claims they have developed just such a device.

To create their device, the researchers started with the idea that it would have to recognize viral DNA rather than circulating antigens. That would allow for the discovery of an infection even before the [immune system](#) got heavily involved. And that led them to begin with loop-mediated isothermal amplification (LAMP) technology to create a point-of-care (POC) device.

It works by concentrating DNA from a pathogen and then bunching it into balls. The balls, the team found, could then be tested using an electrical signaling device, which would identify the unique pathogen. And the number of balls in a sample would provide the degree of concentration of the pathogen.

Testing of the device using saliva samples showed that it was capable of detecting low concentrations of SARS-CoV-2, HIV and the [tuberculosis](#) bacteria. They also found that it could be mass produced inexpensively and that it could be made small enough for sale at virtually any site and used by untrained people. It also returned results in less than an hour.

The device could also be used to detect bacterial enzymes associated with pathogens that are becoming resistant to antibiotics. The researchers plan to continue their research with the goal of trademarking their device and then taking it to market as soon as possible.

More information: Muhammad Tayyab et al, Digital assay for rapid electronic quantification of clinical pathogens using DNA nanoballs, *Science Advances* (2023). [DOI: 10.1126/sciadv.adi4997](https://doi.org/10.1126/sciadv.adi4997)

© 2023 Science X Network

Citation: A simple, low-cost LAMP-based device that can detect low concentrations of pathogens in patient samples (2023, September 7) retrieved 9 May 2024 from <https://medicalxpress.com/news/2023-09-simple-low-cost-lamp-based-device-pathogens.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
