


Long-distance and low-attenuation magnetic energy focusing technology for deep-tissue wireless powering

April 3 2024

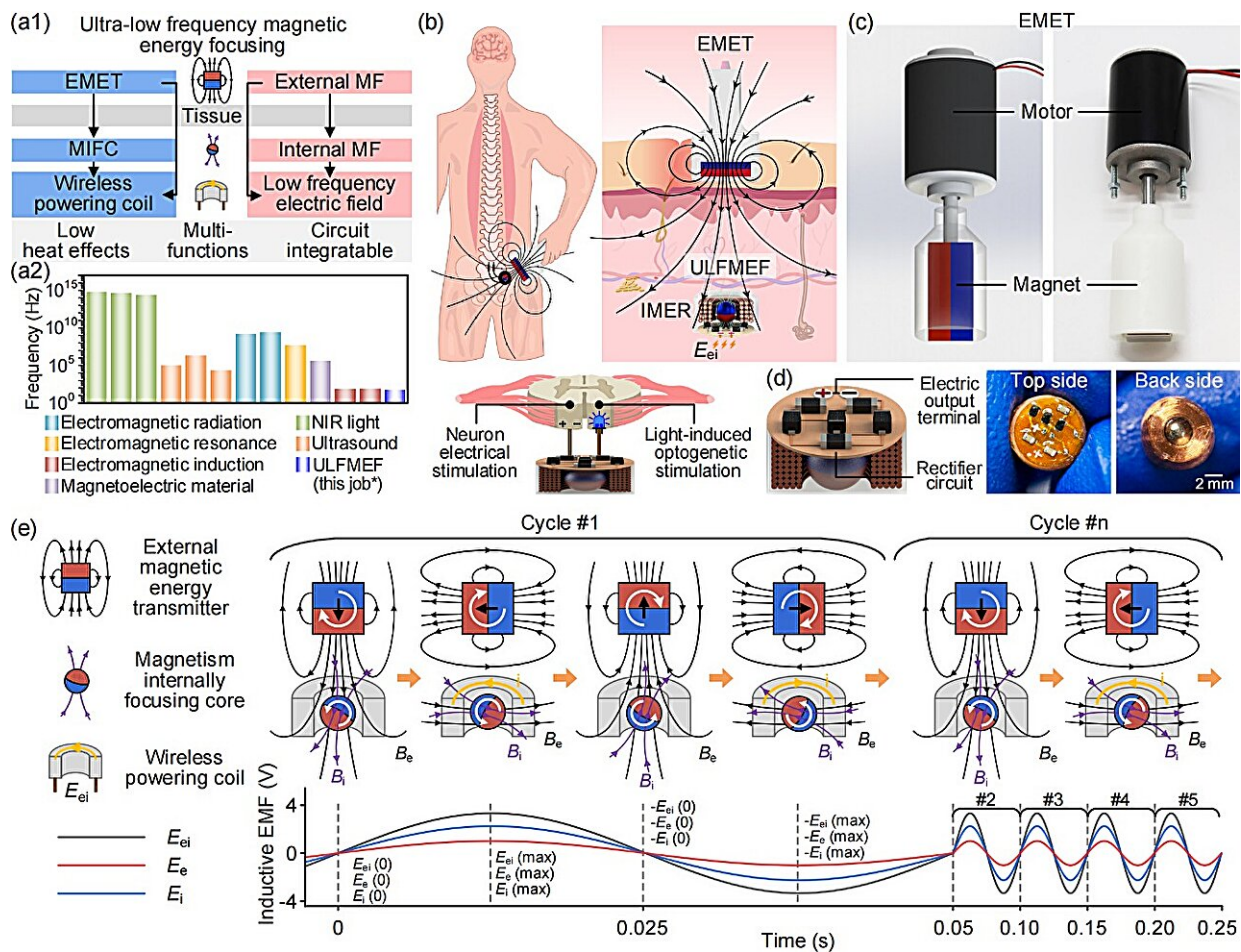

(a1) System design of the ULFMEF developed for wireless charging of implantable electronic devices, where the ULFMEF system consisted of an IMER and an EMET. (a2) Schematic showing the typical working frequency of ULFMEF, compared to other wireless energy transfer such as electromagnetic

radiation, electromagnetic resonance, electromagnetic induction, magnetoelectric material, ultrasound and near-infrared light effects. (b) Illustration of the working mechanism of ULFMEF system applied for wireless electrical stimulation and light-induced optogenetic stimulation in deep tissues. (c) Structure diagram and physical photograph of the EMET, which utilized motor to control the rotation of magnet to generate low-frequency magnetic field. (d) Schematic diagram and photograph of the IMER combined with a rectifier circuit. (e) Schematic diagram showing the external/internal magnetism synergistically electricity generating process in a typical cycle and during multi-cycles. The electricity generated in the IMER through two pathways, including EMET-induced E_e via external pathway and MIFC-induced E_i via internal pathway, respectively. Credit: Science China Press

Fully implantable electronic devices such as cardiac pacemakers, cardiovascular monitors and deep brain stimulators, have been widely developed in medical monitoring, diagnosis, and treatments. Existing implantable devices are based on power supply through replaceable batteries, self-powering supply, and wireless power transfer. The key challenge for disposable batteries is the limited life, which requires intermittent replacement via surgery, resulting in non-negligible health risks and medical costs.

Self-powering supply involves the conversion of endogenous energy in the organism into [electric energy](#) through the circulatory, respiratory, and digestive systems. However, restricted organ movements, weak power, and unstable energy collection also present challenges. By contrast, wireless transcutaneous energy transfer techniques have been developed to transfer external energy to power implanted electronic devices across biological tissues.

Currently, external energy sources, including ultrasound, near-infrared light, heat and magnetic field, have been used for wireless energy

transfer. However, the ultrasound and high-frequency magnetic field can be easily absorbed or reflected by the skin and tissue. The light and heat always result in thermal damage and severe energy attenuation through tissues. Therefore, these techniques generally suffer from issues of low energy transfer efficiency for thicker tissues, while low-frequency (

Writing in *National Science Review*, Prof. Xi Xie and Prof. Lelun Jiang are the first to [propose a methodology](#) of ultra-low frequency magnetic energy focusing (ULFMEF) for highly effective and robust wireless-powering of deep-tissue [implantable electronic devices](#).

The magnetic energy transfer system mainly consists of an implantable magnetic energy receiver (IMER) and a portable external magnetic energy transmitter (EMET). The EMET generates an external magnetic field at ultra-low frequencies and the MIFC generates an internal magnetic field. The combined magnetic fields induce a low-frequency [electric field](#) in the wireless powering coil.

Compared with other [high-frequency](#) technologies, such as the photovoltaic and electromagnetic effects, the ULFMEF system takes advantage of the ultra-low frequency magnetic field with low heat effects and multi-functions. The magnetic-core IMER was fabricated by encapsulating a NdFeB magnetism internally focusing core (MIFC) with high magnetization strength embedded inside a cylinder copper coil, where additional circuits or stimulation electrodes were connected to the wireless powering coils.

The portable magnetic energy transmitter consists of a DC motor coupled to a speed controller to drive the rotation of a NdFeB magnet. The top side and back side of the IMER have a size of $\Phi 8 \times 4 \text{ mm}^3$ and a weight of only $\sim 1 \text{ g}$. A miniature electric circuit was integrated on the top side to rectify the generated E_{ei} -induced alternative current into direct current and boost the voltage.

The portable transmitter can generate a rotating magnetic field at ultra-low frequencies from 5 Hz to 50 Hz via the rotation of the motor-driving NdFeB magnet, where the rotating magnetic field penetrates the biological tissues and induces the electricity of the IMER through two pathways. In the external pathway, the rotating magnetic field of the transmitter can induce a magnetic flux change and generate an external magnetic field-induced electric potential E_e in the coil. Also importantly, in the internal pathway, the MIFC synchronously rotates with the external magnetic field due to the strong magnetic interaction between the driving magnet and MIFC.

This results in the in-situ rotating magnetic field inside the coil and produces the internal [magnetic field](#)-induced electric potential E_i . The total generated electric potential E_{ei} in the IMER consists of the E_e and E_i , where the existence of the MIFC in IMER can remarkably enhance the total output electricity compared to conventional magnetic energy transfer.

In contrast to other wireless energy transfer methods, this ULFMEF methodology significantly increases the transmission distance and slows down the attenuation rate during the energy transfer. Moreover, this low-frequency and long-distance magnetic energy transfer mode of ULFMEF can penetrate the deeper biological tissues with minimal energy loss and thermal damage.

This holds promise for the effective [power supply](#) of implantable microelectronic devices to perform electrical stimulation or optical stimulation in deep tissues. The effective, robust, and versatile features of the ULFMEF render this methodology as a highly promising wireless powering technology for a new generation of fully implantable biodevices.

More information: Yuanyuan Li et al, Ultra-low frequency magnetic energy focusing for highly effective wireless powering of deep-tissue implantable electronic devices, *National Science Review* (2024). [DOI: 10.1093/nsr/nwae062](https://doi.org/10.1093/nsr/nwae062)

Provided by Science China Press

Citation: Long-distance and low-attenuation magnetic energy focusing technology for deep-tissue wireless powering (2024, April 3) retrieved 2 May 2024 from <https://medicalxpress.com/news/2024-04-distance-attenuation-magnetic-energy-focusing.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.